

Pressure **Transmitters**

Typ 4AP-30, 4 AD-30, dTRANS p30. dTRANS p31, 4327, 4341, 4355, 4359, 4362, 4364, 4380

B 40.4300 Operating Instructions

06.02/00350011

Internet: www.JumoUSA.com moo.ASUomuL@ofni E-Mail 6008-086-019 гах OMUL 428-008-1 610-380-8002 Phone Coatesville PA 19320, USA 885 Fox Chase, Suite 103

JUMO PROCESS CONTROL INC.

E-Mail: sales@jumo.co.uk +44 1279 635262 Fax: Phone: +44 1279 635533 Harlow, Essex CM20 2TT, UK Temple Bank, Riverway **JUMO House**

JUMO Instrument Co. Ltd.

Internet: www.jumo.net tən.omu[@lism Phone: +49 661 6003 0 36035 Fulda, Germany Postal adress: 36039 Fulda, Germany Mackenrodtstrasse 14 Delivery adress: 36039 Fulda, Germany Moltkestrasse 13-31

M. K. JUCHHEIM GmbH & Co

Street adress:

1 General

M.K. JUCHHEIM GmbH & Co is a company which is certified according to ISO 9001. The pressure transmitters described below conform to the requirements of DIN and VDE. You have purchased a product which meets even the highest requirements and fulfils, or exceeds, all the spec-

However, if you have any grounds for complaint, please return the instrument to us, with a detailed description of the fault.



Please read these operating instructions before starting up the instrument.

We reserve the right to make technical alterations.

If you have any suggestions for improving these operating instructions, or a product, please ring us at our main factory



Installation notes on the pressure transmitters are included in these operating instructions. If any difficulties should still arise during commissioning or while in operation, please contact your nearest JUMO office or the

Phone: within Germany (0661) 6003-715 from abroad (+49) 661 6003-0 within Germany (0661) 6003-606 (+49) 661 6003-607 from abroad

Internet: www.iumo.net

qualified personnel!

part (2) (see marking on the inner part).

o open up the connector:

★ Unscrew the screw (1).

4.1 Assembly of the terminal box

Terminal box to DIN 43 650, Form A with Pg9 cable gland.

Conductor cross-section up to 1.5 mm² max., external dia.

Terminal box to DIN 43 650, Form C with Pg7 cable gland. Conductor cross-section up to 0.75 mm² max., external

The protection specified will only be achieved when the

connector is firmly in position with the corresponding seal.

of conductor Ø 4.5 - 7 mm, Protection IP65

★ Using a small, flat screwdriver, lever the inner part (3) out of the outer

The inner part can be re-assembled and inserted into the outer part in 4

4.2 Installing the attached connecting cable

Minimum bending radius 120 mm (fixed cable run). The cable must not be compressed. The end of the cable

best to route the cable directly into a switch cabinet. When lengthening the cable, ensure that pressure equilibra-

tion is provided while avoiding the ingress of moisture.

must be located in a dry room to avoid condensation. It is

dia. of conductor Ø 3.5 – 6 mm, Protection IP65.

All the pressure transmitters described in these operating instructions are maintenance-free. They do not contain any components which you could repair or exchange. Repairs can only be carried out at the factory

2 Technical description


These operating instructions do not take into account all possible applications or product variations. If you are looking for notes on your specific application, please contact the main factory.

If you need more detailed technical information on a specific instrument, please ask for the corresponding Data Sheet.

Phone (+49) 661 6003-0

Туре	Data Sheet	Туре	Data Sheet
dTRANS p31	40.2050	4359	40.4359
4327	40.4327	4362	40.4362
4341	40.4341	4364	40.4364
4AP-30	40.4353	dTRANS p30	40.4366
4AD-30	40.4354	4380	40.4380
4355	40.4355		

The instrument version of your pressure transmitter can be seen from the

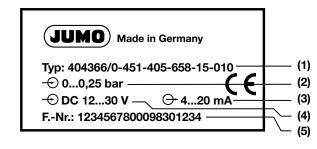

- (1) Type code
- (4) Supply


(5) Serial number

- (2) Range
- (3) Output


4.3 Block/connection diagrams Electrical connection


Pressure transmitters must only be connected by properly

(Output 4 - 20 mA)




Connection with terminal box







4.3.1 2-wire circuit

All components of the measuring circuit are wired in series.



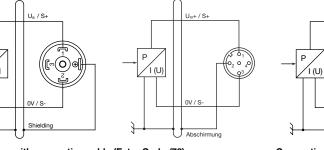

Connection with connecting cable (Extra Code /73)



3 Installation

3.1 Safety note



WARNING

The device does not meet the requirements for a "Components with a safety function" according to the Pressure Equipment Directive 97 / 23 / EC.

For hazardous substances, such as oxygen, acetylene, combustible and toxic materials, as well as in refrigeration equipment, pressure containers etc., the relevant regulations must be followed!

Ignoring these regulations can result in injury or damage to

Only properly qualified personnel may work on this equipment.

3.2 General

The operating position of the pressure transmitter is generally unrestricted. However, in unfavourable circumstances it may falsify the measured

Where there are unusual measurement conditions or media (e.g. high medium temperatures or especially corrosive media), suitable pressure separators from our product range can be used. Our staff will be pleased



Unless otherwise specified, JUMO pressure transmitters have been calibrated vertically with the pressure connection below, at an ambient temperature of 20°C.

For installation in hydraulic plant it is appropriate to mount the pressure transmitter with the pressure connection above, to avoid air pockets.

When using a shut-off device, it should have a progressive opening to ensure a slow increase in pressure. Shut-off devices should be opened slowly to avoid pressure surges.

3.3 Fitting in position


The sealing faces of the pressure transmitter and the measurement point must be protected against dirt and damage. The type and form of the thread which is used at the measurement point is described on the back of the instructions. In case of doubt, please contact the main factory.

The tightening torque depends on the form and material of the seal which is used, and on the pressure connection. The tightening torque should be at least 15 Nm but not more than 200 Nm.


For pressure connections to EN 837 Form B, suitable seals are JUMO

Common minus lead (ground) for supply voltage and measurement


(Output e.g. 0 - 10 V; 0 - 20 mA; 1 - 6 V

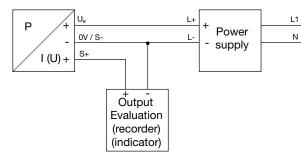

Connection with terminal box



Connection with connecting cable (Extra Code /73)



3.4 Operating conditions ☐ The pressure transmitter must be earthed, and protected against

used to prevent the material seizing up.

available as accessories in our product range

on request.

electrostatic discharges! ☐ The ambient and pressure-medium temperatures must not go

hydraulic seals to DIN 16 258 (flat), as in Data Sheet 40.9700.

For pressure connections to DIN 3852 Form F. JUMO provides the ap-

propriate elastomer seals ex-works, ready-mounted in the pressure con-

Pipe connections to DIN 11 851, DIN 28 403 (KF) and DIN 32 676 (clamp)

include special sealing systems, which can be provided as accessories

For the special pressure connections to the pressure transmitter, with the

Extra Codes /117, /131 and /141, mating connections for welding are

The weld-in mating connection for Extra Code /44 is supplied with the

Taper pressure connections to American standards, such as NPT

threads, are made hand-tight with a spanner. A sealing compound is

- beyond the limits that are given in the corresponding Data Sheet.
- ☐ As for any other sensitive measuring instrument, the pressure transmitter must not be exposed to

excessively large variations in temperature.

- These will eventually cause changes of the zero point and the measu-☐ Do not exceed the measurement range or the permitted overpressu-
- ☐ For highly viscous or crystallizing media which could block the pressure connection, the most suitable versions are those with a frontal
- ☐ The frontal diaphragm must not be deformed under any circumstances - even finger pressure can be enough to cause unacceptable deformation of the diaphragm.
- ☐ Do not insert any objects into the bore of the pressure connection.
- Do not direct a pressure jet onto the diaphragm.
- Under extreme conditions, with rapid changes of pressure and high pressure peaks, snubbers and pressure decoupling elements must be applied, to avoid pressure spikes (water hammer) which would lead to failure of the pressure transmitter.

5 Trouble shooting


.,,,			
	No supply voltage	Check supply voltage	
No output signal	Cable break, incorrect connection	Check connecting cable	
	No input pressure	Check connection to the pressure medium	
	Fault in pressure trans- mitter, caused by imper- missible operating conditions	Return the pressure transmitter to the suppli er, with a detailed de- scription of the fault	
	Measurement system of the instrument has been destroyed by excessive pressure		
Output signal stays constant, even though the pressure chang- es	Output signal from the	Provide the correct sup- ply voltage	
	Output signal from the pressure transmitter is being distorted by the current limiting, resulting from overvoltage	Measurement range is too small – return the pressure transmitter to the supplier, with a de- tailed description of the fault	
	Measurement point is blocked	Check measurement point, if necessary clear or replace it	
	Selected measurement range is too low	Return the pressure transmitter to the suppli er, with a detailed de- scription of the fault	
Output signal too high	The electronics of the pressure transmitter is faulty, or the supply voltage is too high		
Output signal too low	With current output sig- nal: burden is too high With voltage output sig- nal: burden is too low	Change the burden on the measurement circuit	
	Supply voltage is too low	Alter the supply voltage	
Zero of the out- put signal is wrong Output signal	Pressure transmitter measurement has shifted because of impermissi-	Return the pressure transmitter to the suppli er, with a detailed de- scription of the fault	
	ble operating conditions		


Type of fault	Possible cause	Handling	
	No supply voltage	Check supply voltage	
No output signal	Cable break, incorrect connection	Check connecting cables	
	No input pressure	Check connection to the pressure medium	
	Fault in pressure trans- mitter, caused by imper- missible operating conditions	Return the pressure transmitter to the suppli- er, with a detailed de- scription of the fault	
	Measurement system of the instrument has been destroyed by excessive pressure		
Output signal stays constant, even though the pressure chang- es	Output signal from the	Provide the correct sup- ply voltage	
	pressure transmitter is being distorted by the current limiting, resulting from overvoltage	Measurement range is too small – return the pressure transmitter to the supplier, with a de- tailed description of the fault	
	Measurement point is blocked	Check measurement point, if necessary clean or replace it	
Output signal too high	Selected measurement range is too low	Return the pressure transmitter to the suppli- er, with a detailed de- scription of the fault	
	The electronics of the pressure transmitter is faulty, or the supply voltage is too high		
Output signal too low	With current output sig- nal: burden is too high With voltage output sig- nal: burden is too low	Change the burden on the measurement circuit	
	Supply voltage is too low	Alter the supply voltage	
Zero of the output signal is wrong Output signal characteristic is Pressure transmitter measurement has shift because of impermiss ble operating condition (e.g. overpressure)		Return the pressure transmitter to the suppli- er, with a detailed de- scription of the fault	


4.3.2 3-wire circuit


6 Dimensions for pressure connections that are not front-flush

Pressure connection













Threaded bore













7 Dimensions for front-flush pressure connections

Pressure connection










•				
DIN 11851				
DN	D	G	NTS	
20	Ø20	RD 44x1/6	603	
25	Ø26	RD 52x1/6	604	
32	Ø32	RD 58x1/6	605	
40	Ø38	RD 65x1/6	606	
50	Ø50	RD 78x1/6	607	



8 Service

☐ JUMO pressure transmitters do not require any maintenance.

☐ In the event of a fault, there are no components or modules which can be replaced or repaired by the user.

□ Some types of pressure transmitter (Types 4AP-30, 4AD-30, 4355, 4359, 4362/23 and 4364) can be re-adjusted. We recommend that you regularly send in these pressure transmitters to the supplier, as part of your quality assurance

Please return the instrument to the supplier, with a detailed description of the fault.

DIN 32676			
DN	D ₁	D ₂	NTS
20	Ø27.5	Ø34	612
25	Ø43.5	Ø50.5	613
40	Ø45.5		615
50	Ø56.5	Ø64	616

Threaded bore

